

General Specifications

DO30G Sensor for Dissolved Oxygen Analyzer

GS 12J05D03-01E

■ GENERAL

The DO30G sensor for dissolved oxygen is designed for use in water treatment plants such as sewage treatment works, effluent activated sludge process, and potable water treatment. It is also effective in river monitoring, intake protection, fish farming and other fields where water quality is important.

This galvanic cell has a fast response time and good long term stability, and features replaceable diaphragm and cable for easy maintenance. A temperature sensor is incorporated for compensation. The DO30G sensor can be used in either the PB350G/PB360G floating ball holders or in the DOX8HS submersion type holder.



DO30G Sensor



PB350G Floating ball holder


■ FEATURES

DO Sensor with Long-term Stability and Short Electrolyte Stabilization Time

- A DO sensor that uses a special electrolyte, shortening the electrolyte stabilization time and realizing stable measurements over a long period of time.
- Measuring range of 0 to 20 mg/L
- A membrane that is easily replaceable by anyone because of the cartridge type
- A membrane 50 mm thick that is hard to tear and has reduced influence from air bubbles

■ SYSTEM

Refer to GS 12J5D2-E for dissolved oxygen converter DO402G, GS 12A01F02-01EN for 4-wire Converter FLXA402, GS 12A01A03-01EN for 2-wire liquid analyzer FLXA202, GS 12A01A02-01E for 2-wire liquid analyzer FLXA21 and GS 12J05C02-00E for holders.

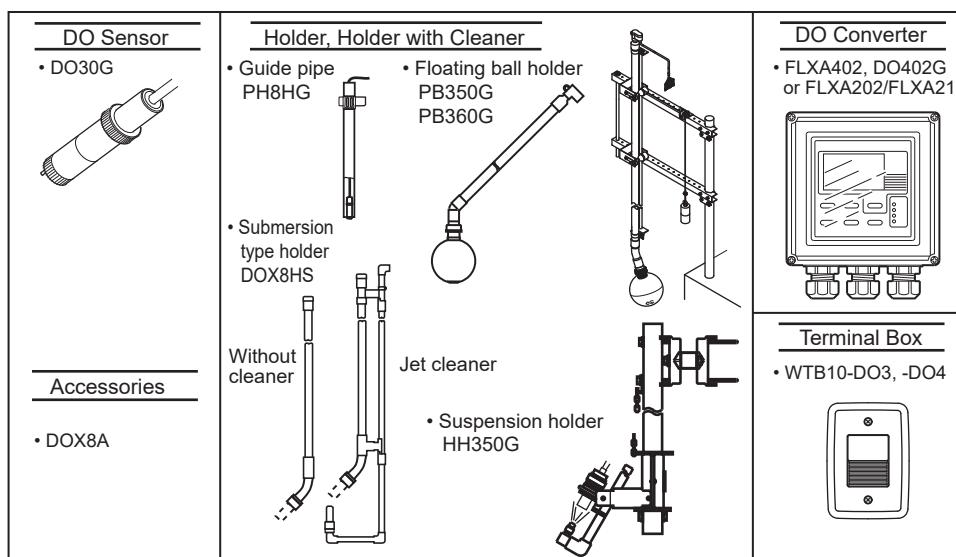

Note: "DO" of DO sensor means dissolved oxygen.

CAUTION



Installation Location of Holders (Guide Pipe, Submersion Type, etc)

The holder should be used in a place that is as vibration free as possible.

Using the holder in a place where it is affected by vibration, may result in damage to the holder.

FLEXA, FLXA, EXADO are registered trademarks or trademarks of Yokogawa Electric Corporation.
All other company and product names mentioned in this GS are registered trademarks or trademarks of their respective companies.

YOKOGAWA ♦

Yokogawa Electric Corporation
2-9-32, Nakacho, Musashino-shi, Tokyo, 180-8750 Japan

GS 12J05D03-01E
©Copyright May. 2007 (YK)
6th Edition: Oct. 2018 (YK)

■ GENERAL SPECIFICATIONS

GENERAL SPECIFICATIONS of DO30G SENSOR

Dissolved Oxygen: 0 to 20 mg/L (ppm)
 Liquid Temperature: 0 to 40°C
 Liquid Pressure: 0 to 100 kPa
 Flow speed: 20 cm/s or more
 Sensor for Temperature Compensation: Pt1000
 Wetted Part Material:
 rigid polyvinyl chloride, stainless steel,
 fluorinated ethylenepropylene, nitrile rubber,
 heat-resistant soft polyvinyl chloride,
 and polycarbonate
 Cable Length: 3 m, 5 m, 10 m, 15 m and 20 m
 Weight: Approx. 0.3 kg + 0.12 × N kg
 N: cable length
 (ex. for cable length of 5 m, approx. 0.9 kg)

CHARACTERISTICS of DO30G SENSOR

Repeatability: 0.1 mg/L or 3% FS, whichever is greater
 (including sensor)
 Temperature Compensation Error:
 Within ±3% FS (including sensor) for a
 ±5°C change in the range of 0 to 40°C
 Response Time: Within 2 minutes
 (90% response)(including sensor)

WTB10 Terminal Box

Used when DO converter is installed at a distance
 from the DO sensor.
 Ambient temperature: -10 to 50°C
 Construction: JIS waterproof
 Case material: Fiberglass reinforced polycarbonate resin
 Electrical connections
 DO sensor side: JIS A8 watertight plastic gland
 DO converter side: JIS A15 watertight plastic gland
 with cable (max. 40 m)
 Conduit adaptor (optional) available
 Case color: Grayish green
 (Munsell 2.5GY5.0/1.0)
 Weight: Body 0.5 kg Mounting hardware: 0.7 kg

DOX8A Parts Set for Maintenance

A set of zero-adjusting reagent and maintenance parts
 <Contents>
 Zero adjusting reagent
 (sodium sulphite 500 g) 1 bottle
 Membrane assembly
 (for membrane thickness of 50 µm) 3 sets
 Electrolyte for sensor (50 mL) 1 bottle
 Syringe for replacing electrolyte 1
 Polish for silver electrode (30 g) 1 bottle
 Polyethylene beaker (200 mL) 1

DOX8W Calibration Set (optional)

This is necessary if the span calibration is to be done
 using a saturated dissolved oxygen solution. It is not
 necessary for air calibration.

<Contents>

Air pump, stirrer, stirring element, bubbler, clamp,
 beaker, and thermometer.

Note: The calibration set can be used in common
 regardless of the type of holder.

■ MODEL AND SUFFIX CODES

1. DO Sensor

Model	Suffix Code	Option Code	Description
DO30G	Dissolved Oxygen Sensor
—	-NN	Always -NN
Membrane thickness	-50	50 µm
Cable length	-03 -05 -10 -15 -20	3 m 5 m 10 m 15 m 20 m
Cable terminal	-PN -FK -FL	Pin terminal (*1) Fork terminal M4 ring terminal (*2)

*1: Select pin terminal for FLXA402, DO402G, DO202,
 and FLXA202/FLXA21.

When terminal box is used, select WTB10-DO3.

*2: Used to connection to FLXA202/FLXA21.
 When terminal box is used, select WTB10-DO4.

2. Terminal Box

Model	Suffix Code	Option Code	Description
WTB10	Terminal box
Combined system	-DO3 -DO4	For FLXA402, DO402G,DO202, and FLXA202/FLXA21 (*1) For FLXA202/FLXA21 (*2)
—	-NN	Always -NN
Specify cable length	-00 -05 -10 -20 -30 -40	No cable 5 m 10 m 20 m 30 m 40 m
Option	Mounting hardware /P /W /AWTB /ANSI	Pipe mounting hardware Wall mounting hardware G 1/2 1/2NPT
Conduit work adaptor			

*1: Used for pin terminals, and cable with pin terminals.

*2: Used for M4 screw terminals, and cable with M4 ring terminals.

3. Accessories (parts set for maintenance)

Model	Suffix Code	Option Code	Description
DOX8A	Parts set for maintenance (for membrane thickness of 50 µm)
Sensor	-M	For membrane replacing type sensor
—	*B	Style B

4. Calibration Set

Model	Suffix Code	Option Code	Description
DOX8W	*A	Calibration set

5. Spare Parts


Part Name	Part No.	Remarks
Membrane and electrolyte for sensor	K9171HK	3 membrane assemblies (thickness of 50 µm) 50 mL of electrolyte Syringe for replacing electrolyte
Zero adjusting reagent	L9920BR	Sodium sulfite 500g
Polisher	K9088PE	For polishing silver electrode 30g

■ DIMENSIONS


DO Sensor DO30G

Unit: mm


Dissolved-oxygen sensor with pin terminals

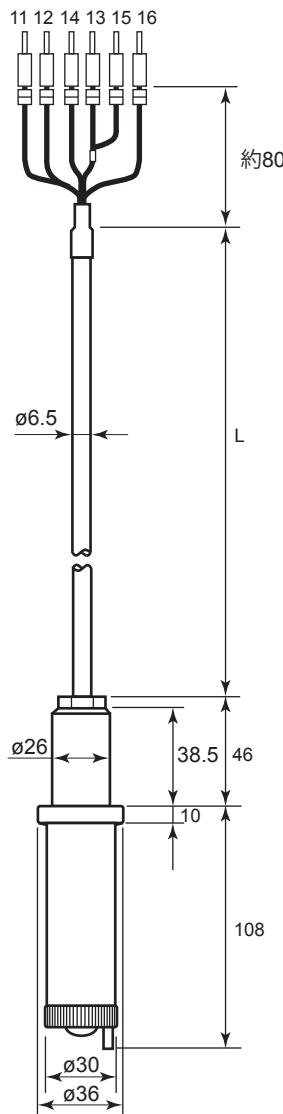

Dissolved-oxygen sensor with fork terminals

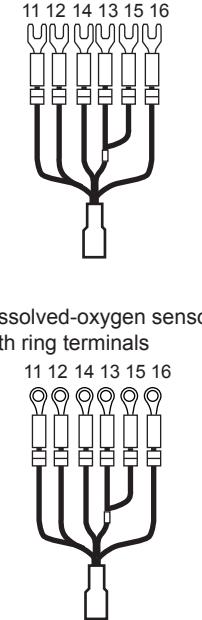

Dissolved-oxygen sensor with ring terminals



Terminal assign

13	IE
15	RE
11	T1
12	T2
14	Shield
16	Liquid earth

Pin terminals

Model and Suffix Codes	L	Weight (kg)
DO30G - NN - 50 - 03 - PN	3 000	Approx. 0.6
DO30G - NN - 50 - 05 - PN	5 000	Approx. 0.8
DO30G - NN - 50 - 10 - PN	10 000	Approx. 1.4
DO30G - NN - 50 - 15 - PN	15 000	Approx. 2.0
DO30G - NN - 50 - 20 - PN	20 000	Approx. 2.6

Fork terminals

Model and Suffix Codes	L	Weight (kg)
DO30G - NN - 50 - 03 - FK	3 000	Approx. 0.6
DO30G - NN - 50 - 05 - FK	5 000	Approx. 0.8
DO30G - NN - 50 - 10 - FK	10 000	Approx. 1.4
DO30G - NN - 50 - 15 - FK	15 000	Approx. 2.0
DO30G - NN - 50 - 20 - FK	20 000	Approx. 2.6




Ring terminals

Model and Suffix Codes	L	Weight (kg)
DO30G - NN - 50 - 03 - FL	3 000	Approx. 0.6
DO30G - NN - 50 - 05 - FL	5 000	Approx. 0.8
DO30G - NN - 50 - 10 - FL	10 000	Approx. 1.4
DO30G - NN - 50 - 15 - FL	15 000	Approx. 2.0
DO30G - NN - 50 - 20 - FL	20 000	Approx. 2.6

F02.ai

Terminal Box WTB10

Unit: mm

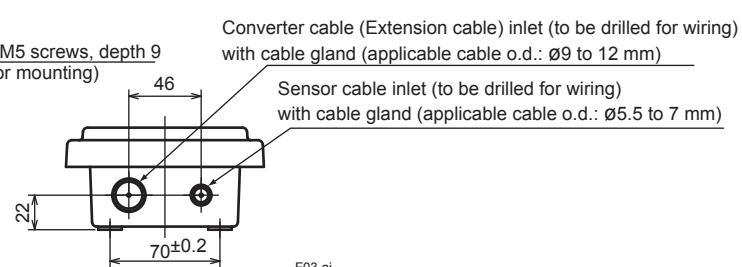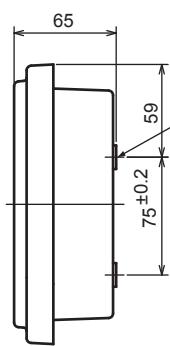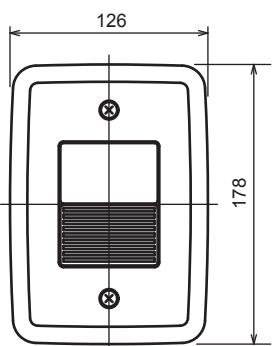


Converter cable (Extension cable) inlet (to be drilled for wiring)
with cable gland (applicable cable o.d.: Ø9 to 12 mm)

Sensor cable inlet (to be drilled for wiring)
with cable gland (applicable cable o.d.: Ø5.5 to 7 mm)

F03.ai


Detailed drawing of cable gland for terminal box

Unit: mm

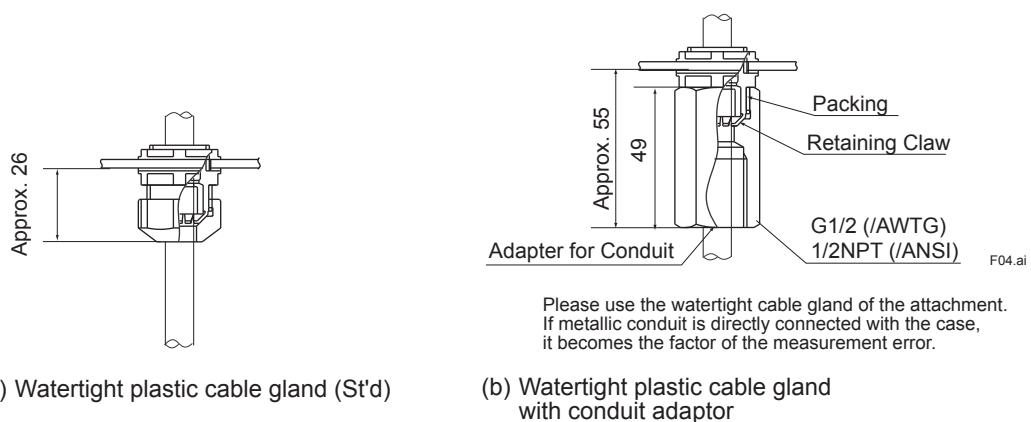


Dedicated Extension Cable with WTB10 (Not supplied if suffix code “-00” is selected)

Unit: mm

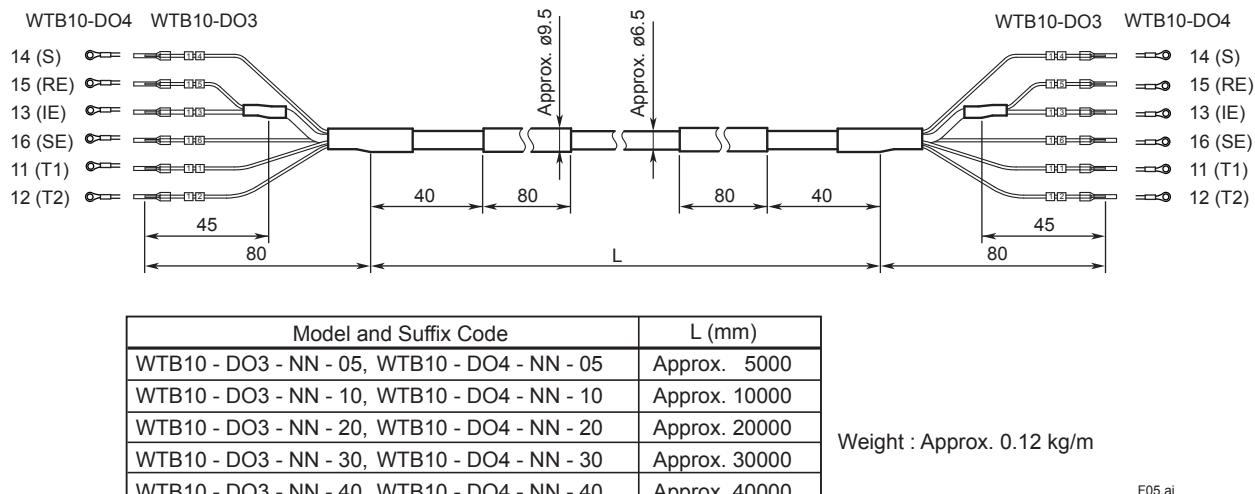


Pipe Mounting Bracket (Optional) (Option Code: /P)

Unit: mm

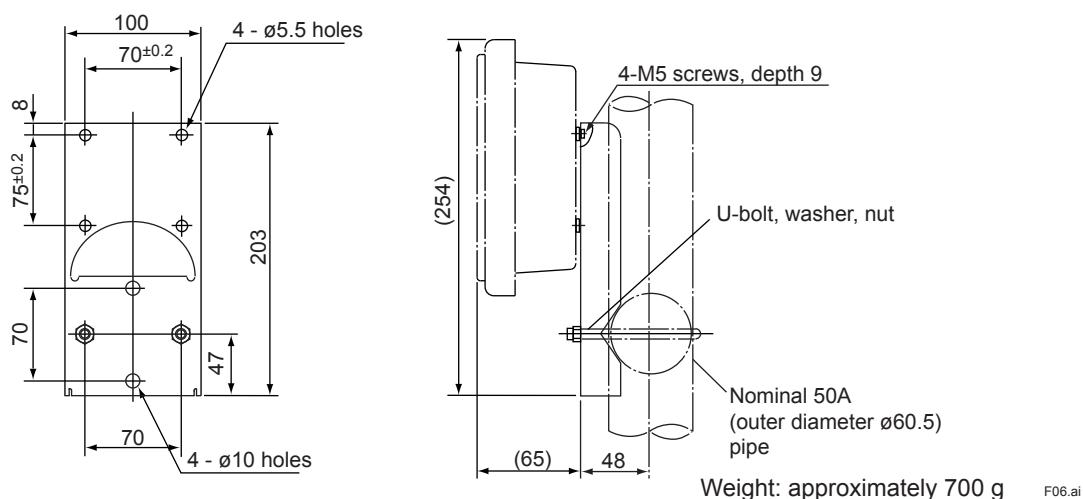


Wall Mounting Bracket (Optional) (Option Code: /W)

Unit: mm

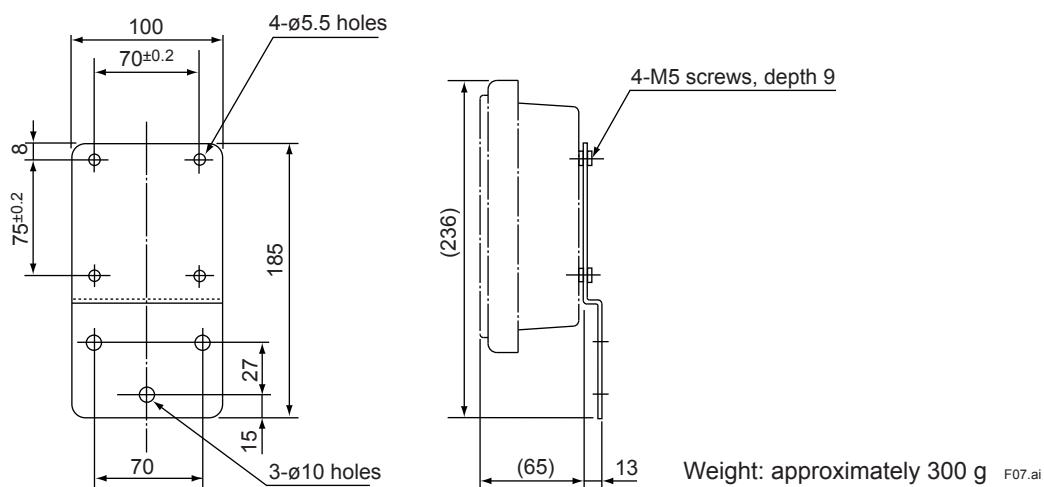

■ WIRING DIAGRAM EXAMPLE

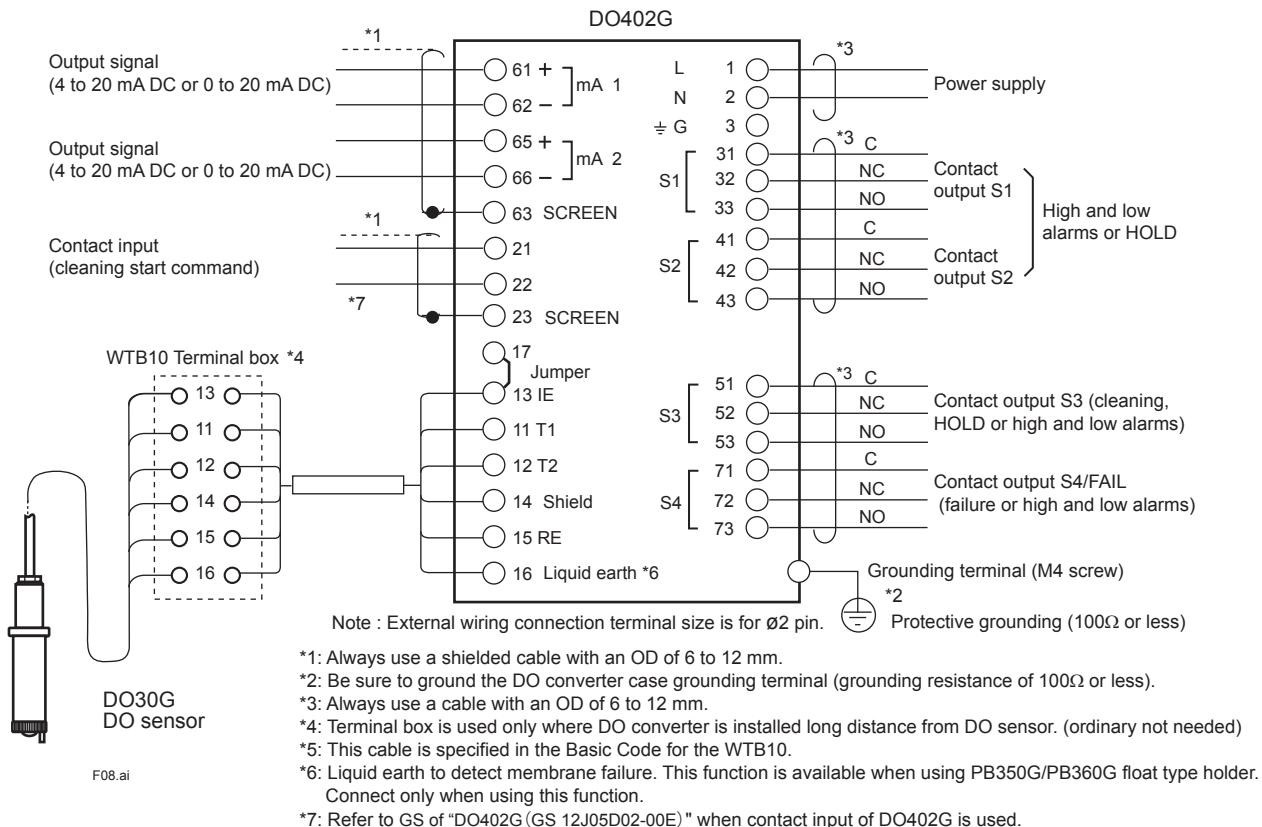

Inquiry Specifications Sheet for Dissolved Oxygen Analyzer

For inquiries on the Yokogawa dissolved oxygen analyzer, please tick (✓) the appropriate box (□) and write down the relevant information in the blanks.

1. General

Name of your company: _____
Name of person : _____ Dept. or sect : _____ (Phone No.)
Name of plant : _____
Measuring point : _____
Purpose of use : Indication Recording Alarm Control
Power supply : _____ V AC _____ Hz DC _____

2. Measurement Conditions

(1) Liquid temperature : _____ to _____, Normal [°C]
(2) Liquid pressure : _____ to _____, Normal [kPa]
(3) Flow speed : _____ to _____, Normal [m/s]
(4) Name of liquid to be measured : _____
(5) Components of liquid to be measured : _____
(6) Other conditions : _____

3. Installation environment

4. Requirements

(1) Measurement range : 0 to 20 mg/L _____

(2) System component selection: Sensor Holder Converter Cleaning system Calibration set
 Parts set for maintenance Terminal Box

(3) Length of sensor cable : 3 m 5 m 10 m 15 m 20 m

(4) Type of holder : Guide pipe Submersion Floating ball Suspension

(5) Cleaning method : No cleaning Jet cleaning

(6) Other requirements :